
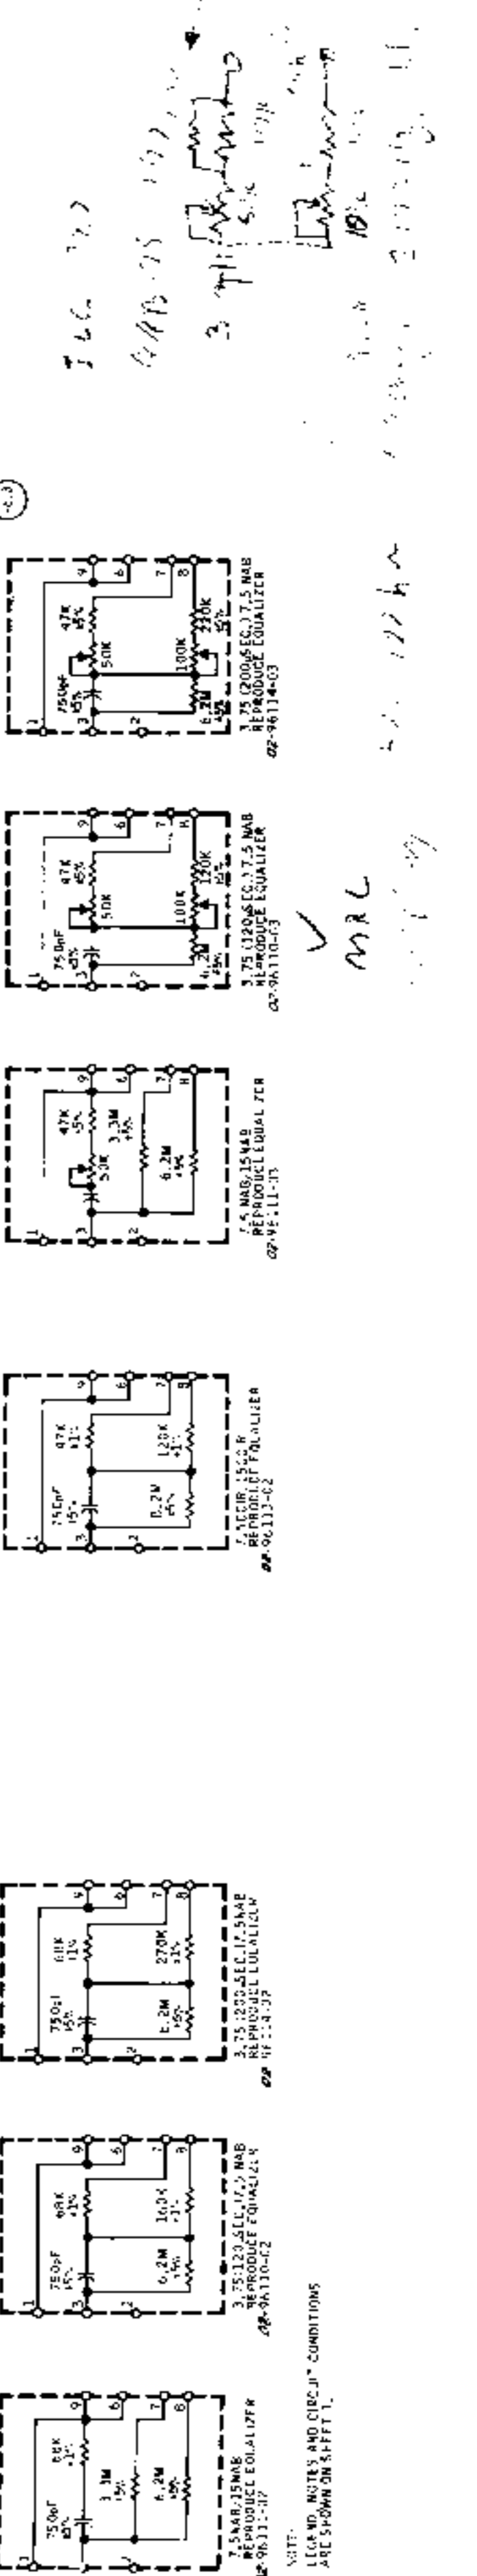


Ac values -

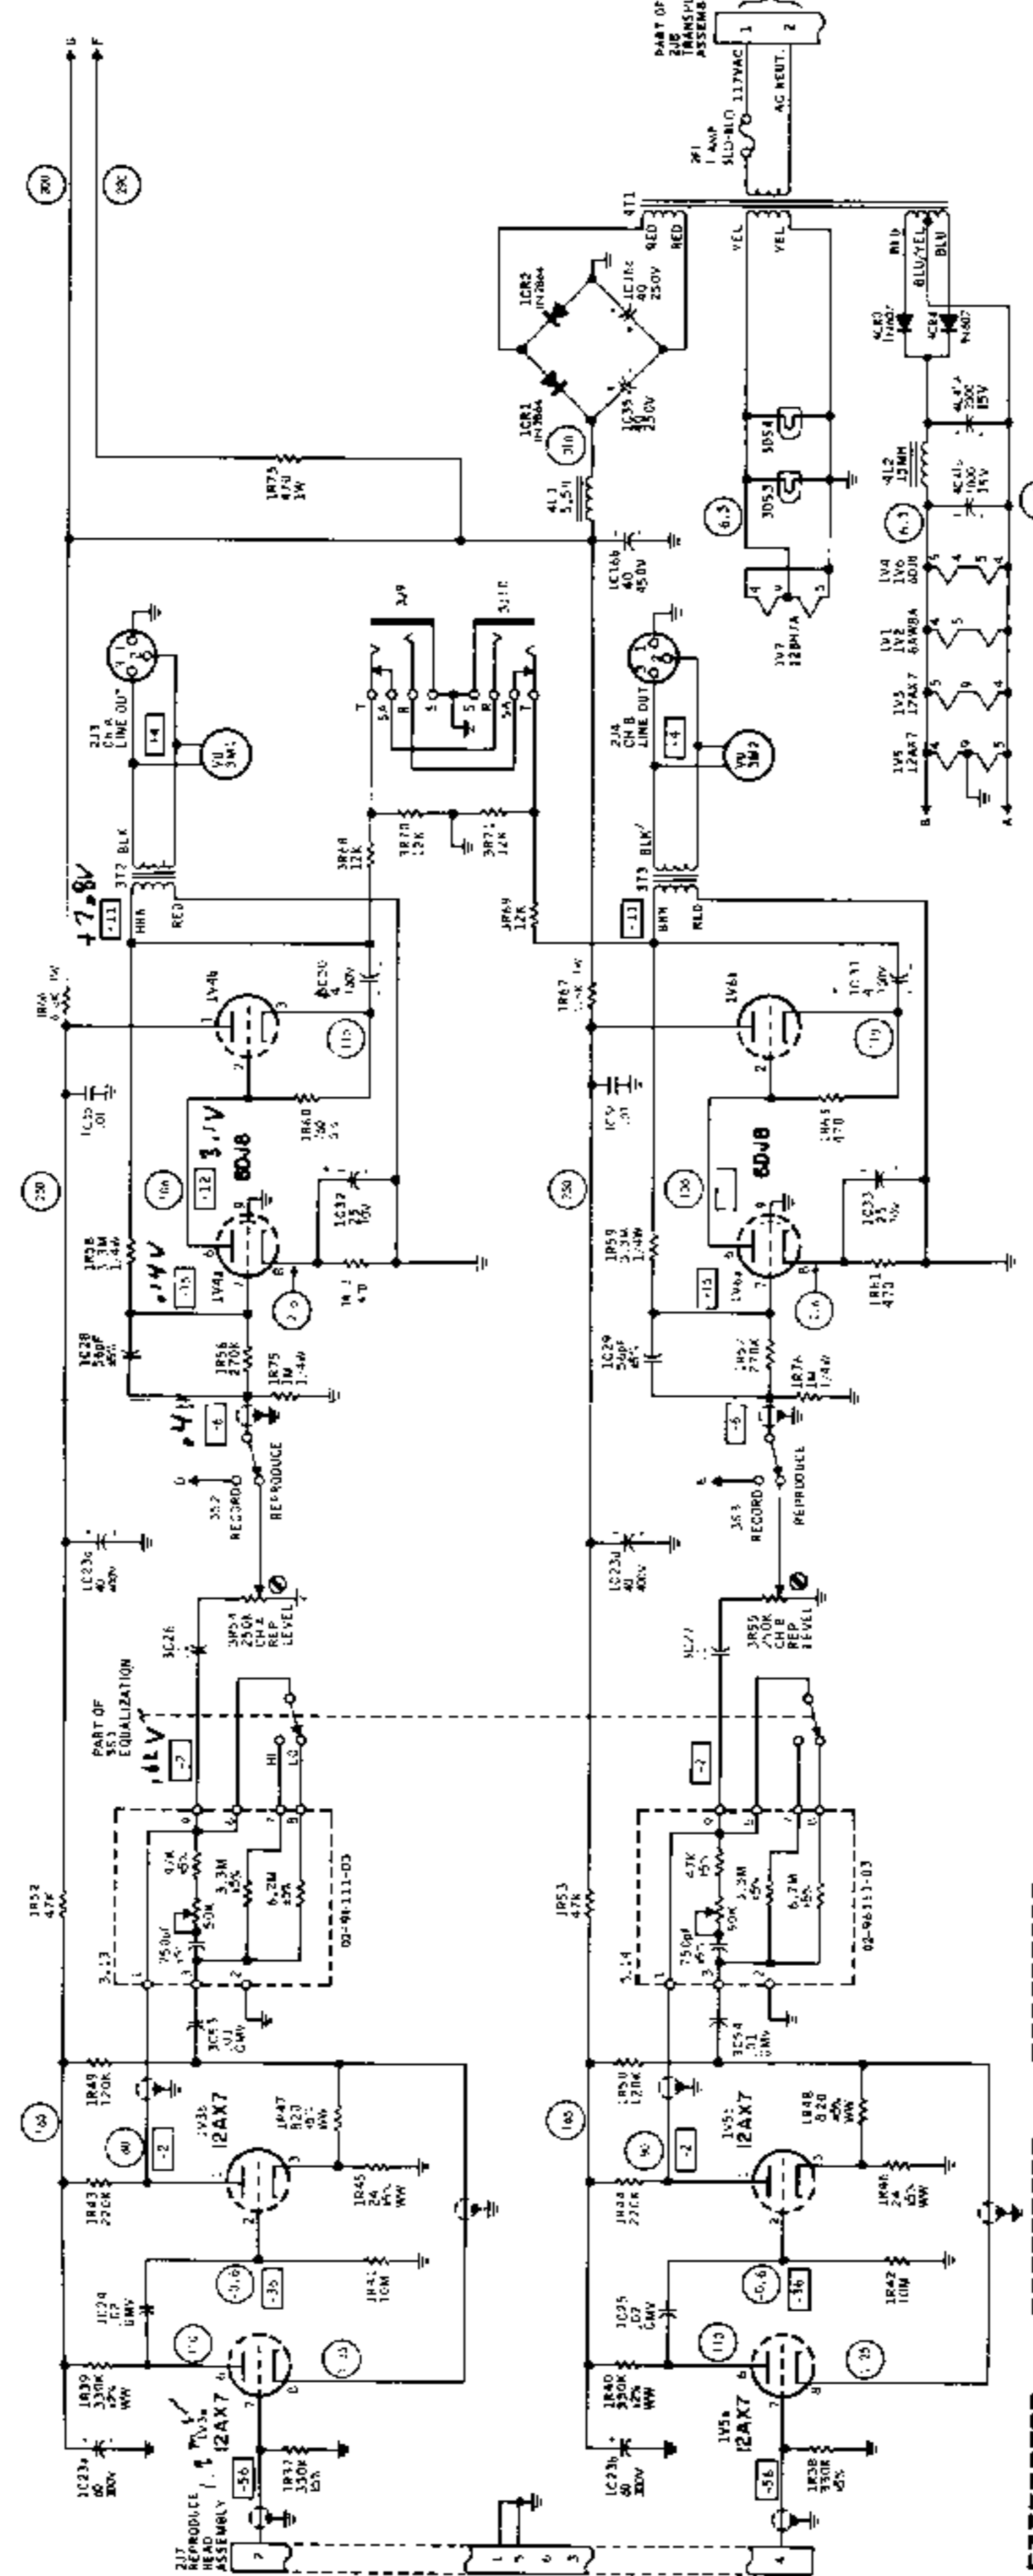

Handwritten notes and signatures:

MRC
3166 322
3166-35 197
3 371-1
1878
REPRODUCE EQUALIZER
281 1 AMP 5LD-BLO 117VAC
REPRODUCE EQUALIZER
281 1 AMP 5LD-BLO 117VAC
REPRODUCE EQUALIZER
281 1 AMP 5LD-BLO 117VAC
REPRODUCE EQUALIZER
281 1 AMP 5LD-BLO 117VAC
REPRODUCE EQUALIZER
281 1 AMP 5LD-BLO 117VAC

NOTE:
LEG. NO. NOTES AND CIRCUIT CONDITIONS
ARE SHOWN ON SHEET 1.